



**FIG. 1A**

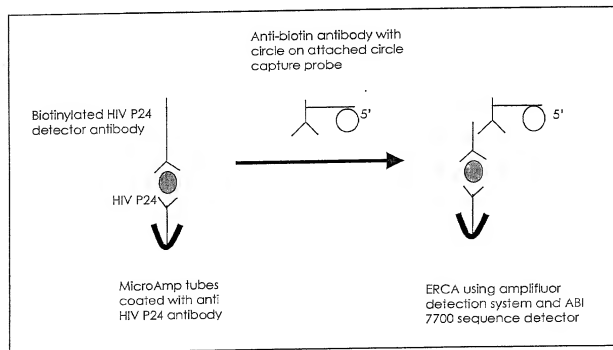


**FIG. 1B**

208020-9982/001


# Coating of microtitre plates and microamp tubes with anti-biotin antibody

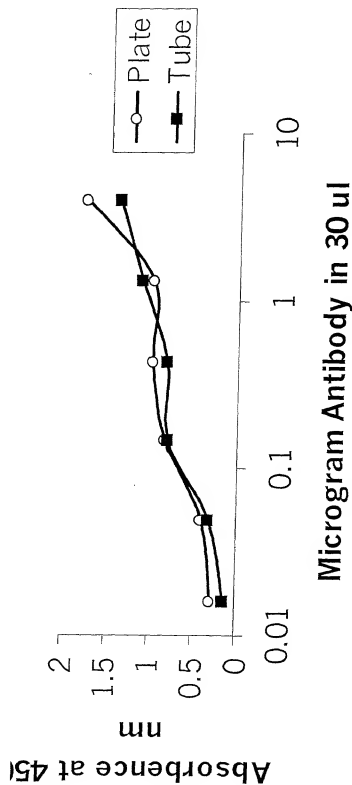

**FIG. 2**

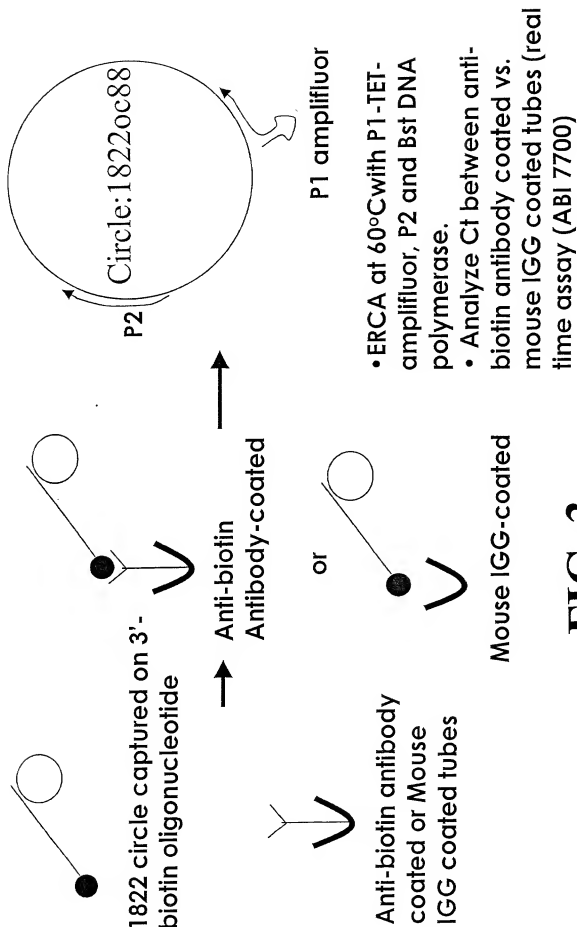

# FIG. 3

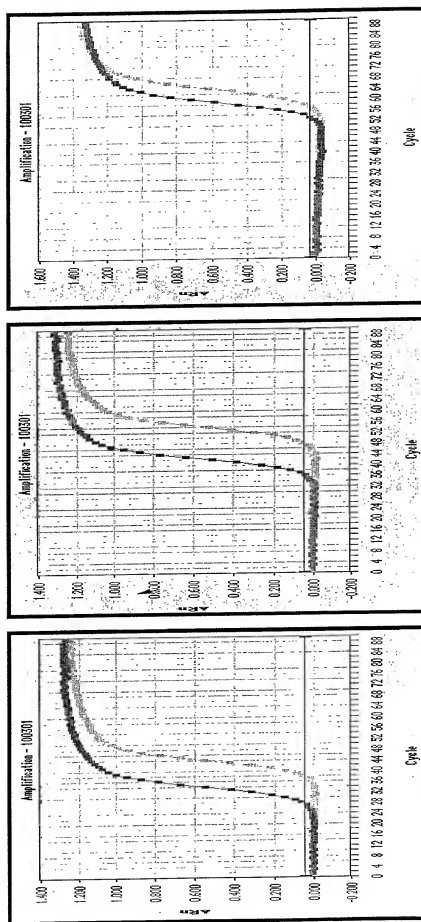


48 x 10<sup>6</sup> circles  
 $\Delta$  Ct = 20 min

1 x 10<sup>6</sup> circles  
 $\Delta$  Ct = 18 min

360 circles  
 $\Delta$  Ct = 10 min


Dark trace = MicroAmp tubes coated with anti-biotin antibody  
 Light trace = MicroAmp tubes coated with mouse IGG

FIG. 4

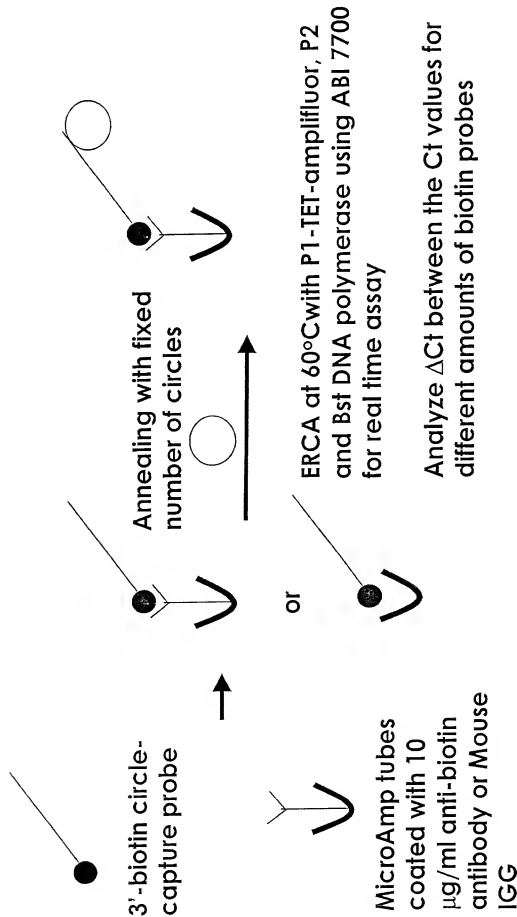


**FIG. 5**

208020'99927001

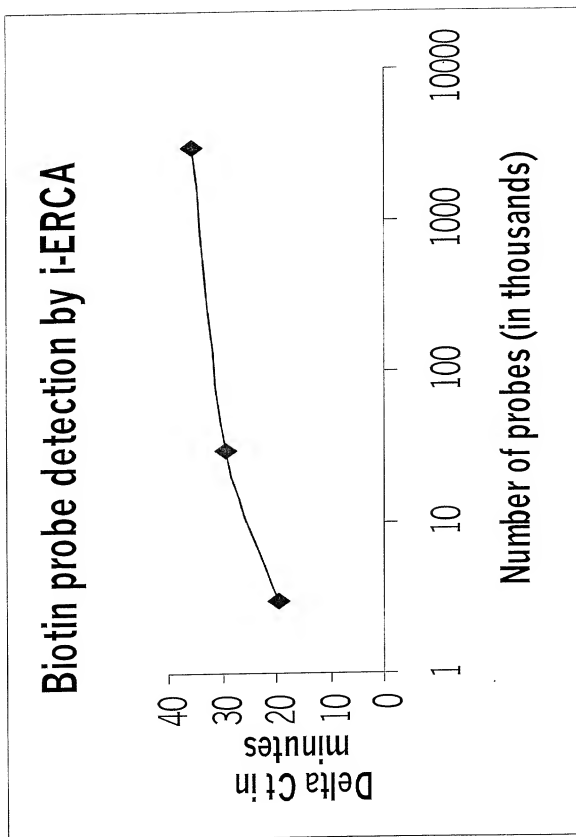


**FIG. 6**

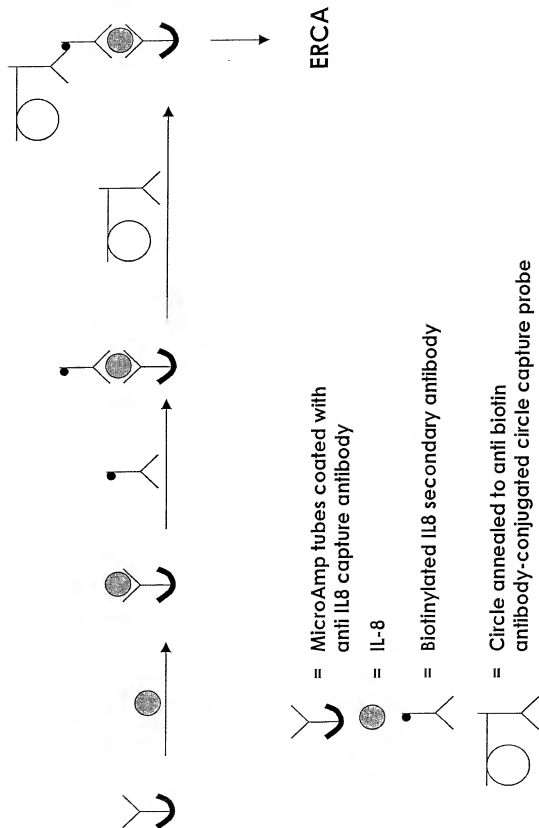

**FIG. 7**

208020-93924001

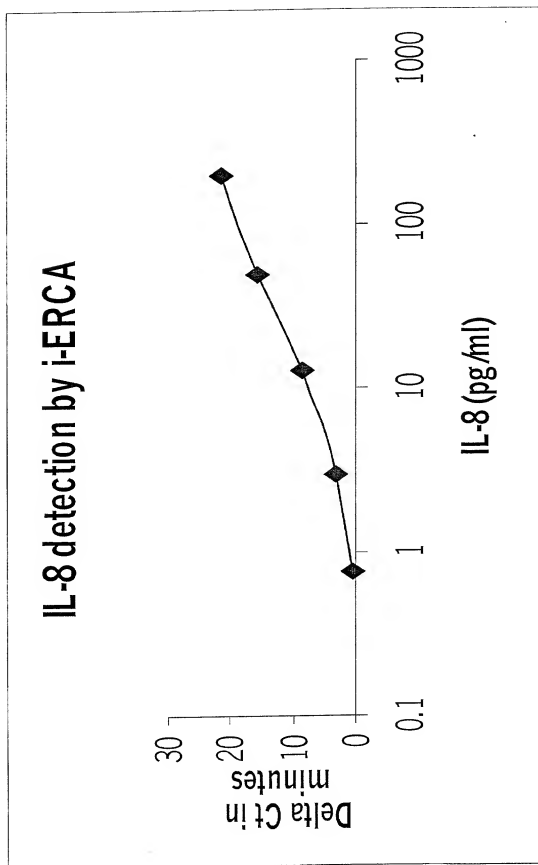

**FIG. 8**

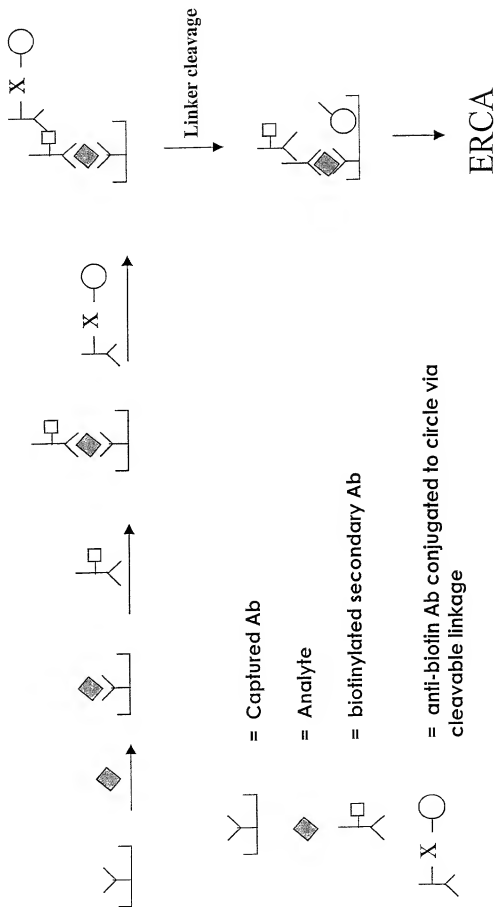


FIG. 9